


The UpLift Support Sling


Warnings and Instructions: Review carefully, proper application is required

⚠ Warning: This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.


Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

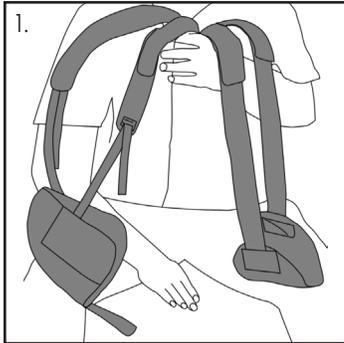


1. Place sling with elbow cuff on impaired side of patient. Hold "O" ring and separate straps.

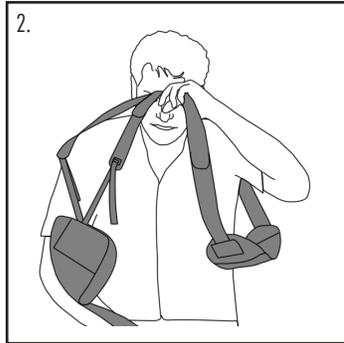


2. Place elbow of unaffected arm between front and back straps of wrist cuff.

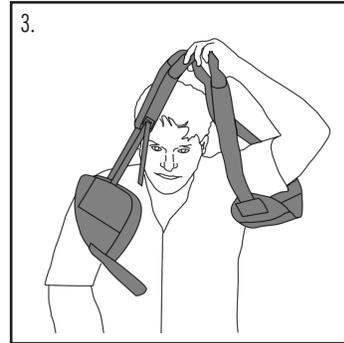


3. Lift "O" ring over head allowing "O" ring to rest on back of neck.

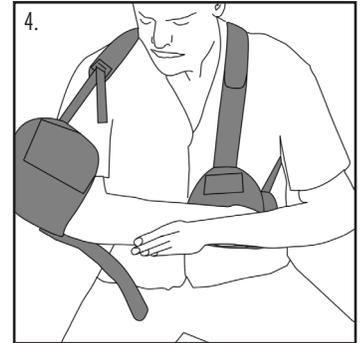


4. Place the wrist of the impaired arm into the wrist cuff.

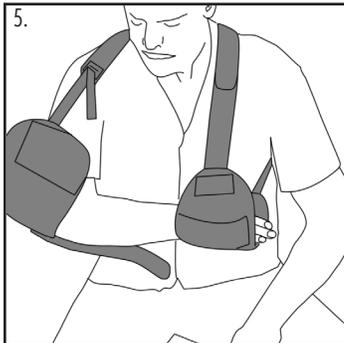


5. Place the elbow of the impaired hand into the elbow cuff. Align the wrist and the elbow cuffs.

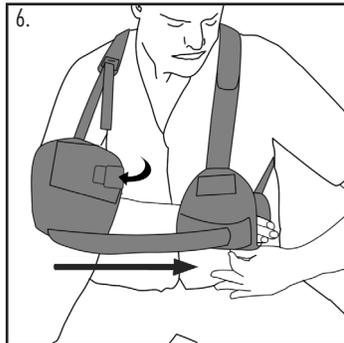

6. Pull the strap that is attached to the elbow cuff and fasten to the wrist cuff. Attach and fasten the bicep strap around the arm on the elbow cuff.

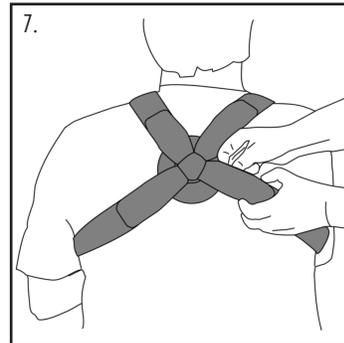

7. The practitioner can make final strap adjustments as needed for proper fit.

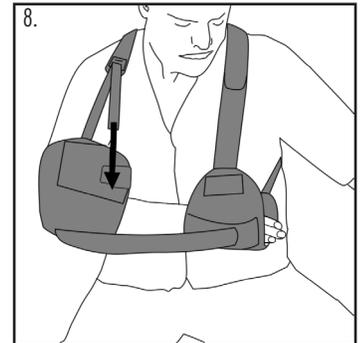


8. Pull the lift strap to comfortably adjust the resting position of the arm.

OPTIONAL: Application of Swathe Strap



9. Attach the end of the swathe strap having the "O" ring connector to the front of the elbow cuff. Face the "O" ring and swathe strap toward the outside of the impaired side of the patient.

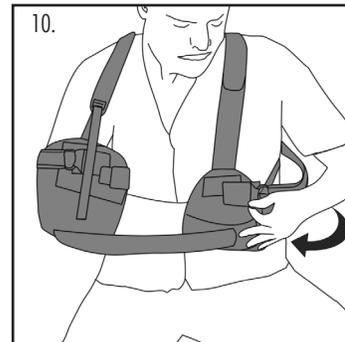

10. Pull the loose end of the swathe strap around the back of the patient and fasten the loose end of the swathe strap to the front of the wrist cuff.